

N E W

HORIBA
Automotive Test Systems

Micro Dilution Tunnel
MOLT-ONE
Partial Flow Dilution Sampling System



 **HORIBA**
ONE
PLATFORM

Explore the future

Automotive Test Systems | Process & Environmental | Medical | Semiconductor | Scientific

HORIBA

MDLT-ONE

The MDLT-ONE is designed to sample particulate emissions using the partial flow dilution method. A small portion of the total exhaust is diluted with HEPA* filtered air to create a constant flow rate through particulate filters to collect Particulate Matter (PM). Compliant to the latest regulations, the new MDLT-ONE is very compact and offers faster response by the use of high precision venturi flow meters and a piezo actuated valve.

* HEPA : High Efficiency Particulate Air

Features

- **Small package**

Heated filter system and flow controllers installed in a single rack. Swivel connection of tunnel section to cabinet allows flexible installation.

Auto filter changer* can also be mounted in the main rack for space efficiency.

- **Automatic calibration software enhances accuracy and ease of use**

The MDLT-ONE series performs automatic calibration by flowing air in-series through the two venturi flow meters and correcting any difference to zero in the software. This can be included into an automated sequence within a test template.

- **Integrated Operating Platform**


HORIBA ONE series systems employ a common user interface, "HORIBA ONE PLATFORM" offering future expandability and ease of integration into Test Automation Systems.




* Please contact HORIBA, when you ordering

Applications

PM Emission Measurement of All Engines

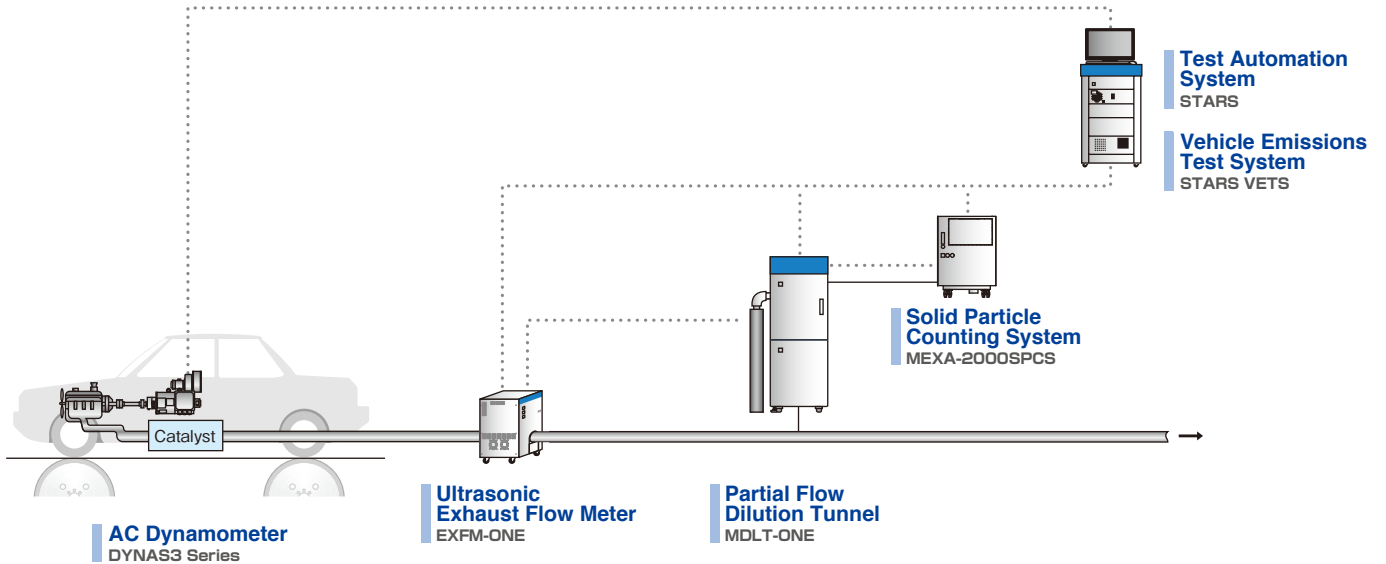

R&D Support of Engine and After Treatment System

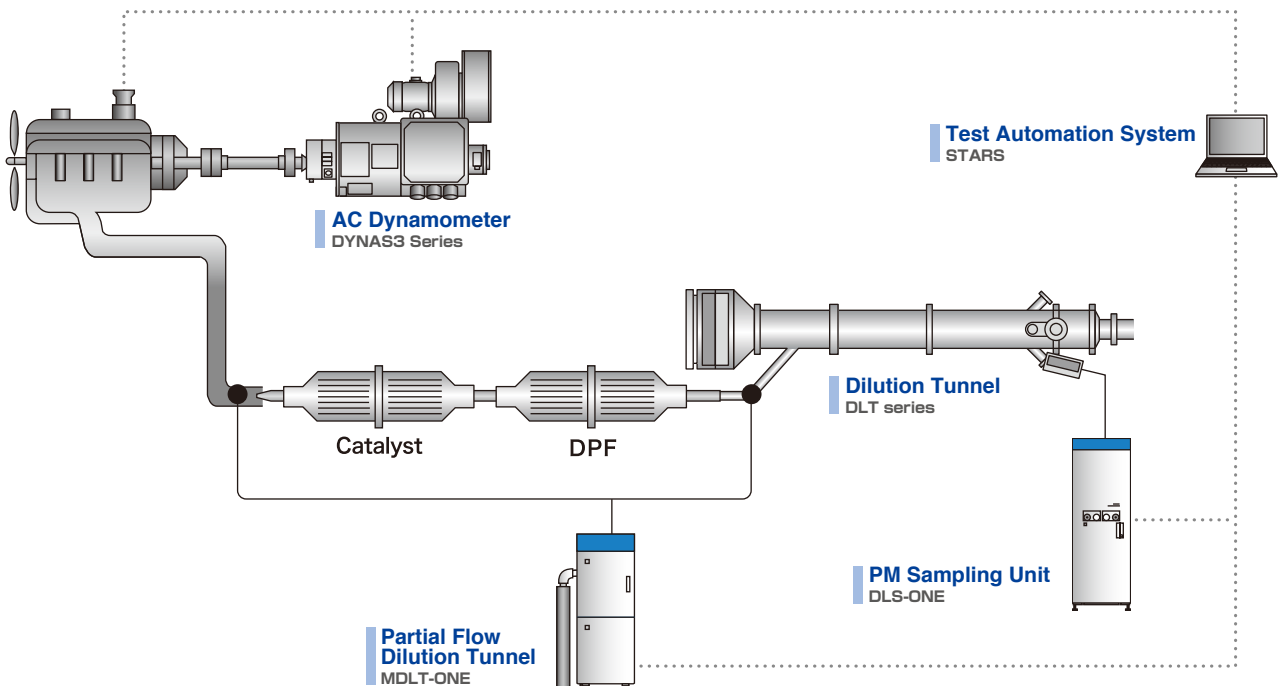

Complies with worldwide emissions regulations

ISO-16183

Japan: Post post new long term

EU: Euro VI (HDV)

EU: Stage IV / V (NRMM)

US: 40 CFR Part 1065/1066

Specification

System outline	
PM sampling method	Partial flow dilution method
Control modes for dilution	Proportional sampling mode (Const. split ratio)/ Fixed dilution ratio mode (Const. dilution ratio)/ Fixed flow rate mode (Manual control)
Control methods for dilution	<ul style="list-style-type: none"> Real-time control based on analog input of exhaust flow rate Control based on learned pattern of exhaust rate
Required signal for gas sampling	Isolated analog signal (0 to 10 V)
Flow rate of diluted gas	35 to 80 L/min*1 (under the condition of 20 °C and 101.3 kPa)
Accuracy of dilution ratio	Within ± 5 % (excluding the system with AFIC) When dilution ratio=15 rate at 20 °C and 101.3 kPa : 35 to 80 L/min
PM mass calculation*2	PM mass (in g/test, g/h or g/kWh) can be calculated and saved, based on integrated values of flow rated and dilution ratio.
Configurations	
System configuration	<ul style="list-style-type: none"> Main unit : Dilution-tunnel unit Operation unit : PC, monitor, keyboard and mouse (table is not included)
Utilities	Purified air : for dilution gas, 400 to 700 kPa, oil free, at least 120 L/min (at 20 °C and 101.3 kPa)
Power supply voltage and frequency	<ul style="list-style-type: none"> Main unit : 100/110/120/200/220/230/240 V AC, 50/60 Hz, single phase Operation unit : 100/110/120 V AC, 50/60Hz or 200/220/230/240 V AC, 50 Hz, single phase
Power requirements	Main unit : Max. 3.0 kVA / Operation unit: Max. 0.5 kVA
Dimensions	<ul style="list-style-type: none"> Main unit : 570 (W) x 730 (D) x 1700 (H) mm Space for operation unit : 900 (W) x 500 (D) mm (table is not included)
Mass	Main unit : Approx. 300 kg (excluding operation unit)
Number of filter lines	Max. 6 lines (5 for sample, 1 for bypass)
Type of filter holder	<ul style="list-style-type: none"> φ70 mm type : actual PM sampling area φ60 mm, with back-up filter φ47 mm type : actual PM sampling area φ37 mm*1, with back-up filter*1
Operating conditions	
Sampling Pressure	Between atmospheric pressure and up to 40 kPa Back pressure of exhaust line : Less than 1 kPa
Options	
Filter auto-changer*3	Changer for automatic replacement of PM filter (φ 47 mm), both single-filter method and multi-filter method are available.
Valve switching	Additional air valve before filter (Replacement of sampling filter on bypass mode)
HOST interface*3	LAN communication using a 10 Base T port Conforms to IEEE802.3 (ISO880 2/3)
Conditioner for dilution air / Compressor	

*1, For the filter face velocity in the regulations (less than 100 cm/s), the flow rate for the φ47 mm filter must be 65 standard L/min.

*2, Input the amount of PM collected on filter to calculate PM mass. It is necessary to input engine output (kW) to calculate the PM mass engine output (g/kWh).

*3, Please contact HORIBA, when you ordering.

IMS The HORIBA Group adopts IMS (Integrated Management System) which integrates Quality Management System ISO9001, Environmental Management System ISO14001, and Occupational Health and Safety Management System OHSAS18001. We have now integrated Business Continuity Management System ISO22301 in order to provide our products and services in a stable manner, even in emergencies.



Please read the operation manual before using this product to assure safe and proper handling of the product.

- The specifications, appearance or other aspects of products in this catalog are subject to change without notice.
- Please contact us with enquiries concerning further details on the products in this catalog.
- The color of the actual products may differ from the color pictured in this catalog due to printing limitations.
- It is strictly forbidden to copy the content of this catalog in part or in full.
- The screen displays shown on products in this catalog have been inserted into the photographs through compositing.
- All brand names, product names and service names in this catalog are trademarks or registered trademarks of their respective companies.

<http://www.horiba.com> e-mail: info@horiba.co.jp

HORIBA, Ltd. Japan

Head Office
2 Miyahonogashi, Kisshoin, Minami-ku, Kyoto, Japan
Phone: 81 (75) 313-8121 Fax: 81 (75) 321-5725

Tokyo Sales Office
2-6, KandaAwaji-cho, Chiyoda-ku, Tokyo, 101-0063, Japan
Phone: 81 (3) 6206-4721 Fax: 81 (3) 6206-4730

HORIBA (China) Trading Co., Ltd. China

Unit D, 1F, Building A, Synnex International Park, 1068 West Tianshan Road, Shanghai, 200335, China
Phone: 86 (21) 6289-6060 Fax: 86 (21) 6289-5553

Beijing Branch
12F, Metropolis Tower, No.2, Haidian Dong 3 Street, Beijing, 100080, China
Phone: 86 (10) 8567-9966 Fax: 86 (10) 8567-9066

HORIBA Instruments (Singapore) Pte Ltd. Singapore

3 Changi Business Park Vista #01-01 Akzonobel House, Singapore 486051
Phone: 65 (6) 745-8300 Fax: 65 (6) 745-8155

HORIBA Vietnam Co., Ltd. Vietnam

Unit 6, 10 Floor, CMC Tower, Duy Tan Street, Dich Vong Hau Ward, Cau Giay District, Hanoi, Vietnam
Phone: 84 (24) 3795-8552 Fax: 84 (24) 3795-8553

PT HORIBA Indonesia Indonesia

Jl. Jalur Sutera Blok 20A, No.16-17, Kel. Kunciran, Kec. Pinang Tangerang-15144, Indonesia
Phone: 62 (21) 3044-8525 Fax: 62 (21) 3044-8521

HORIBA (Thailand) Limited Thailand

East Office
850 / 7 Soi Lat Krabang 30 / 5, Lat Krabang Road, Lat Krabang, Bangkok 10520, Thailand
Phone: 66 (0) 2734 4434 Fax: 66 (0) 2734 4438

HORIBA KOREA Ltd. Korea

202-501, Bucheon Techno Park, 388, Songnae-Daero, Wonmi-Gu, Bucheon-Si, Gyeonggi-Do, 14502, Korea
Phone: 82 (32) 621-0100 Fax: 82 (32) 621-0105

HORIBA India Private Limited India

246, Okhla Industrial Estate, Phase 3 New Delhi-110020, India
Phone: 91 (11) 4646-5000 Fax: 91 (11) 4646-5020
Technical Center
D-255, Chakan MIDC Phase-II, Bhamboli Village, Pune-410501, India
Phone: 91 (21) 3567-6000

HORIBA Instruments Incorporated USA

9755 Research Drive, Irvine, CA 92618, U.S.A.
Phone: 1 (949) 250-4811 Fax: 1 (949) 250-0924
Ann Arbor Facility
5900 Hines Drive Ann Arbor, MI 48108 U.S.A.
Phone: 1 (734) 213-6555 Fax: 1 (734) 213-6525

TCA/HORIBA Sistema de Testes Automotive Ltda. Brazil

Rua Goiás 191 Vila Oriental, Diadema, São Paulo, Brazil CEP 09941-690
Phone: 55 (11) 4224 0200 Fax: 55 (11) 4227 3133

HORIBA UK Limited UK

Northampton Office
Kyoto Close Moulton Park, Northampton NN3 6FL, UK
Phone: 44 (1604) 542-500 Fax: 44 (1604) 542-699

HORIBA Test Automation Limited UK

Teme House, Whittington Hall, Whittington Road, Worcester, WR5 2RY, UK
Phone: 44 (1905) 359-359 Fax: 44 (1905) 359-332

HORIBA Europe GmbH Turkey

Istanbul Office
Küçükbakkalköy Mah. Kayışdağı Cad., Flora Residence No:3 / 2504 34750 Ataşehir / İstanbul
Phone: (90) 216 572 1166 Fax: (90) 216 572 1167

HORIBA FRANCE SAS France

Les Ulis Office
12. Av des Tropiques Hightec Sud, F-91955 Les Ulis, France
Phone: 33 (1) 69-29-96-23 Fax: 33 (1) 69-29-95-77

HORIBA OOO Russia

Altufievskoe shosse, 13, building 5, 127106, Moscow, Russia
Phone: 7 (495) 221-87-71 Fax: 7 (495) 221-87-68

HORIBA Europe GmbH Germany

Hans-Mess-Str.6 D-61440 Oberursel Germany
Phone: 49 (6172) 1396-0 Fax: 49 (6172) 1373-85

HORIBA Europe Automation Division GmbH Germany

Zabergaeustr. 3, D-73765 Neuhausen, Germany
Phone: 49 (7158) 933-300 Fax: 49 (7158) 933-399

HORIBA Europe GmbH Sweden

Sweden Branch (Sodertalje)
Sydhamnsvagen 55-57, SE-15138, Sodertalje, Sweden
Phone: 46 (8) 550-80701 Fax: 46 (8) 550-80567

HORIBA ITALIA SRL Italy

Torino Office
Via Ferroggio, 30, 10151 Torino, Italy
Phone: 39 (11) 904-0601 Fax: 39 (11) 900-0448

HORIBA Czech Czech

Prague Office
Prumyslova 1306 / 7, CZ-10200, Praha 10, Czech Republic
Phone: 420 (2) 460-392-65

HORIBA (Austria) GmbH Austria

Kaplanstrasse 5 A-3430 Tulln, Austria
Phone: 43 (2272) 65225 Fax: 43 (2272) 65230